


### CoaDATA 2001



- Measuring principle: Turbidensitometry
- Process: Single or double determinations
- Reagent block: Heated to 37 degrees C  
2 measuring cells with magnetic stir motor  
1 heated & stirred reagent position  
3 heated not stirrer reagent positions  
18 cuvette incubation positions
- Light protection cap: Integrated pipette guide
- Cuvette: Micro cuvette
- Test volume: 150 ul to 300 ul
- Display: Liquid Crystal Display
- Control panel: Membrane keypad
- Memory: A max. of 7 test methods can be stored
- Conversions: PT (sec) in %, ratio, INR,  
Fibrinogen (sec) in g/l or mg/dl
- Calibration curve: memory of 9 meas. points / assay
- ChipCard (optional): Optional memory board upon request with test specific data such as lot no., calibration curve, preselection for test application for PT, aPTT, TT, Fibrinogen, and others.
- Port I/O: RS-232C
- Power supply: adjustable voltage 110 VAC or 220 VAC
- Weight: approx. 2.3 lbs.
- Size: 10.75" wide x 13.60" deep x 4.9" high

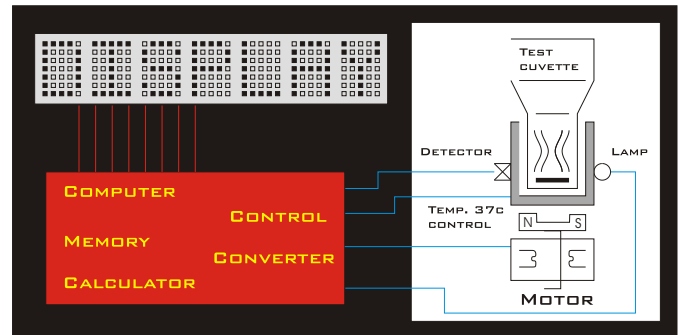

**Distributed in the USA by:**  
**American LAbor**  
 1308 Broad Street  
 Durham, NC 27705

Voice 919-286-0726  
 Fax 919-286-3956  
 Tech. 800-424-0443  
[www.americanlabor.org](http://www.americanlabor.org)